



General

The medical gas wall outlets shall be Powerex Ohmeda compatible quick connect medical gas outlets. Medical gas outlets shall be manufactured in an ISO 9001 facility. Wall outlet shall be designed for concealed piping installation and available for services indicated.

Outlet shall be provided complete with a gas specific rough-in assembly, gas specific latch valve assembly, and a trim plate. Outlet shall be cleaned for Oxygen use. All assemblies shall be 100% tested for leaks, manufactured to comply with the latest edition of NFPA 99, and UL Listed.

Latch Valve Assembly

The latch valve assembly shall be Ohmeda compatible quick connect and accept only gas specific Ohmeda type quick connect adapters. Each latch valve assembly shall be color-coded for ease of gas identification per NFPA 99 standards. Latch valve assemblies shall have gas specific pin indexing corresponding to the rough-in assembly to prevent interchangeability of gas services and is adjustable up to 1" for variations in wall thickness.

Materials used in latch valve assembly: aluminum,

zinc alloy, ABS plastic, steel/brass+plating, stainless steel, brass, neoprene, rubber.

Rough-in Assembly

Universal rough-in assembly shall include the wall rough-in plate (16 ga.) with inlet tubing silver brazed to the outlet body. Inlet tubing shall be type "K" copper, 1/2" (12.7 mm) OD, extend 7-3/4 inches (165 mm), and swivel 360° for ease of installation. Rough-in assembly shall accept only the specified gas service by use of indexes. Rough-in assembly shall be of modular design to permit on-site ganging of multiple outlets with assurance of accurate alignment and providing 5" centerline spacing. A dust plug and cover shall be provided to protect rough-in assembly from contamination during handling and installation at the job site. Materials used in rough-in assembly: stainless steel, ABS plastic.

Rough-in assemblies shall accept any latch valve assembly of the same gas service. The latch valve assembly shall be interchangeable, allowing conversion from one connection style to another without shutting down the medical gas system.

All positive pressure gas outlets shall have a primary and secondary check valve, where the secondary valve in the rough-in assembly allows servicing of the latch valve assembly without having to disrupt gas service to the outlet.

Trim Plate

The standard trim plate provided with the outlet shall be cast aluminum, powder coated chrome, and shall attach with the latch valve assembly to the rough-in assembly. Alternate trim plate of cast aluminum, powder coated grey, shall be available upon request.

MRI Compatibility


MRI compatible models are available (see ordering information chart) and are made with non-ferrous metals.

Ordering Information

Gas Service	Wall Outlet	MRI Outlet
Oxygen	OLET-WALL-OHM-O2	OLET-WALL-OHM-O2-MRI
Medical Air	OLET-WALL-OHM-AIR	OLET-WALL-OHM-AIR-MRI
Medical Vacuum	OLET-WALL-OHM-VAC	OLET-WALL-OHM-VAC-MRI
Nitrous Oxide	OLET-WALL-OHM-N2O	OLET-WALL-OHM-N2O-MRI
WAGD	OLET-WALL-OHM-WAGD	OLET-WALL-OHM-WAGD-MRI
Carbon Dioxide	OLET-WALL-OHM-CO2	OLET-WALL-OHM-CO2-MRI

Additional Options	Part Number
Slide	OLET-SLIDE
Slide	OLET-SLIDE-MRI
Alternate Trim Plate	TRIM-GREY

Dimensions

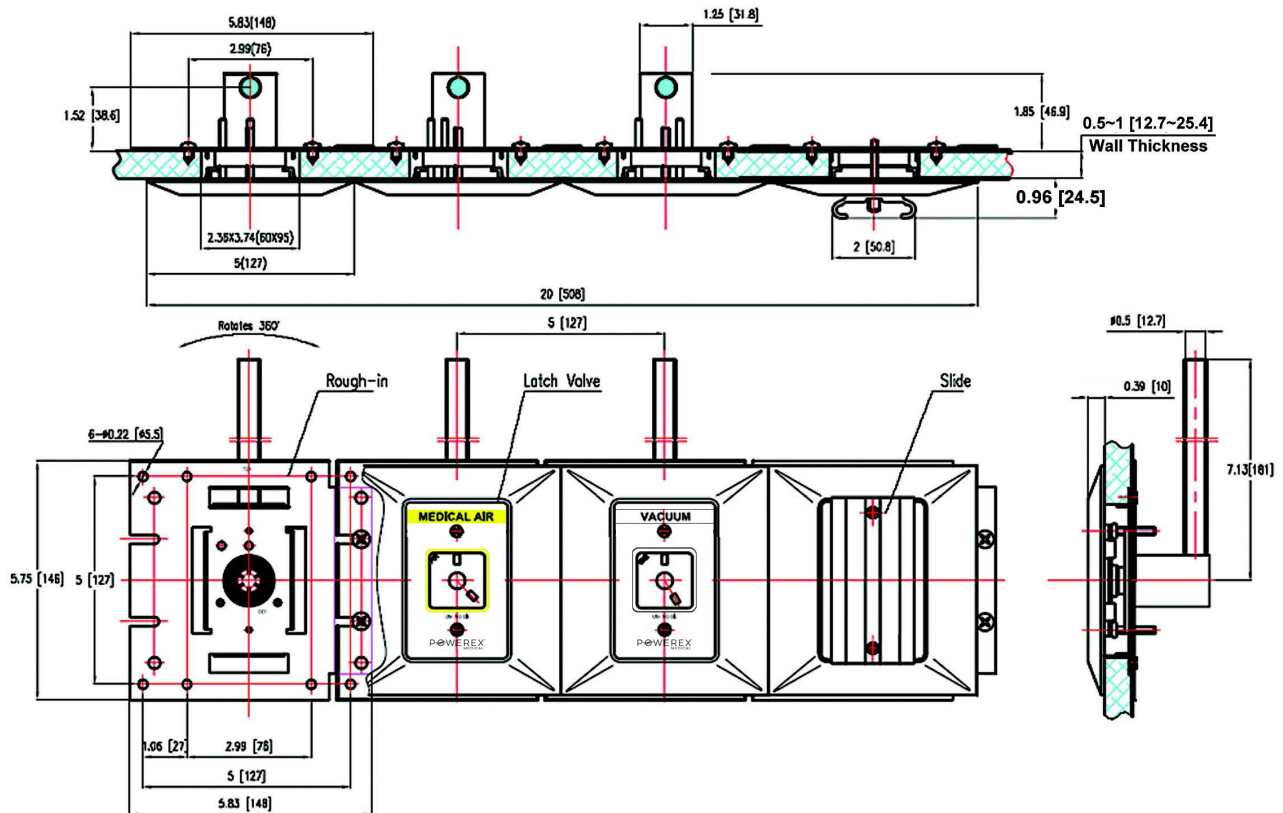

Notes

1. Inch (mm)
2. Additional support needed if ganging more than 3 outlets
3. Wall thickness may vary from 1/2" to 1" (12.7 mm to 25.4 mm)
4. 1/2" O.D. (3/8" Nominal) type K cooper inlet tube allows 360° swivel on outlet body for entry from any angle